

You've been fired!

Flammability standards put to the test

Pressure care equipment (mattresses and cushions) has been tested for years using furniture flammability test standards. This article discusses why these standards are less appropriate for medical devices these days, and what has been developed for cushion flammability testing to replace the furniture tests.

As a result of marked increase in UK fire-related deaths in the home from the 1960s to the late 1980s, the UK Government took action through the introduction of the Furniture and Furnishings (Fire) (Safety) Regulations 1988 (amended 1989 and 1993). These regulations cover different testing needed for fillings, fabrics, and composites, and include match-flame and cigarette tests. (FIRA has an excellent set of guidelines that can be downloaded from their website¹.)

Pressure care equipment registered as medical devices have been the subject of considerable debate. It is an offence for 'domestic' beds (i.e. beds for private use in the home) to be supplied in the UK if they contain fillings which do not comply with the 1988 Furniture and Furnishings Regulations. Compliance entails the need for those fillings (foam and non-foam) to resist ignition as specified in the Regulations. There is, however, a legal anomaly. Beds and cushions that are registered as 'medical devices' appear to be allowed, within the law, to be supplied to the British consumer even if the items in question do not comply with the Regulations. The justification for treating 'medical device' beds and cushions as being exempt from the Regulations is that such items need to comply with medical device regulations instead.

With the limited availability of medical-devices-specific flammability testing, most regulatory requirements have nevertheless turned to Furniture testing. However, whereas the Furniture Regulations select a single type of test depending on the material and usage, the medical devices world has fallen down on requiring both a flame and a cigarette test be carried out. There are International, European, and British (e.g. BS 71772) furniture flammability standards that are each very similar, with only small differences, such as timings.

'Cigarette' tests

The starting point for the Part 10 tests was that cushions should meet a minimum flammability standard. Furniture's cigarette test was a starting point, but labs in the US and Germany found that there was enormous variation in the heat output from different cigarettes from any one pack, and thus this was not a standardised heat source, set aside the health risks of using tobacco based products.

In addition, cigarettes in this century have changed from those available when the furniture standards were originally drafted: 'Fire Safe' requirements are now in place, where a cigarette not being allowed to continue burn when left, have changed the burn characteristics. Therefore, for the Part 10 testing, a 'virtual' cigarette was developed using a heated rod as a heat source, with a required heat output curve to mimic that of an original lighted cigarette (Fig 1).

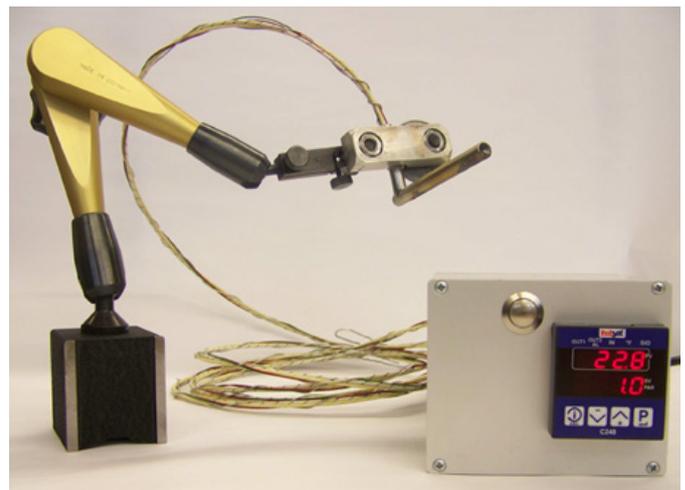


Figure 1. The surrogate cigarette used for ISO 16840-10 flammability testing

Since then, other heat sources have been trialed, such as an electric blow torch (where the air blown on the test sample affected the rate of burn) and an IR heat source (but the results differed if the test material were reflective (e.g. white) or not (e.g. black)).

What looks promising for future iterations is a NiCr coil, which can also have the current adjusted to mimic different heat sources, potentially from 'cigarette' to 'Crib 7' (Fig 2).

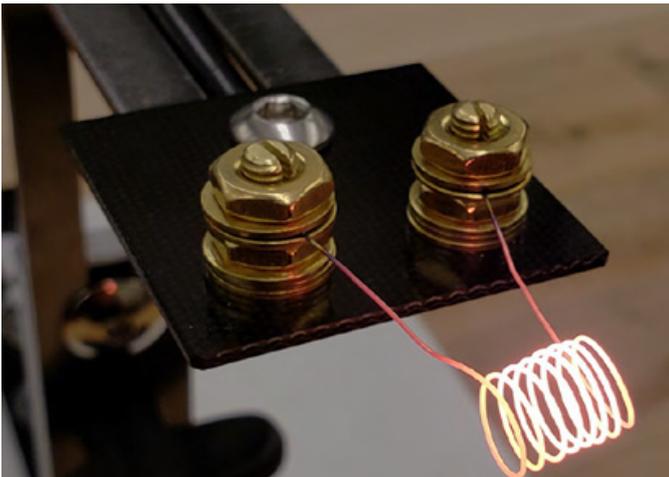


Figure 2. A simple NiCr coil heat source to mimic the burning area of a cigarette

So what's new?

In the United States, data collected back in the 1990s showed that only a small number of individuals per million wheelchair users had died due to fire⁴, and smoking has decreased strongly since then. Public FDA records indicate most 21st century flammability incidents involving wheelchairs have been from electrical faults⁵.

Thus, the current view is that wheelchair cushion design should be focused on tissue integrity, body positioning, and functionality, and not be overly hampered by flammability concerns. California bedding flammability regulations have in 2019 been made less stringent, dropping the need there for a flame test.

In line with this trend, ISO 16840-10 has been adapted to cover all postural support devices on a wheelchair, in addition to just the original seat and back supports. Test set-up designs have

been modified to cover smaller items than were originally provided for. This revision of Part 10 is at the International DIS voting stage at present, and should be published in full later this year.

Have you checked whether the items you are handling have been tested to current medical device standards, rather than to Furniture standards?

PS A parallel standards Working Group is looking to see to what extent the concepts and applications in the wheelchair seating standard might be applied to mattresses, to enable their testing to move away from Furniture flammability standards as well.

1. <https://www.fira.co.uk/images/FIRA-Flammability-Guide-PDF-with-links.pdf>
2. BS 7177 Specification for resistance to ignition of mattresses, mattress pads, divans and bed bases.
3. ISO 7176-14:2008 Wheelchairs — Part 14: Power and control systems for electrically powered wheelchairs and scooters — Requirements and test methods
4. Calder, CJ, & Kirby, RL (1990) Fatal wheelchair related accidents in the United States Am J Phys Med Rehabil 64, 184-190
5. <https://www.accessdata.fda.gov/scripts/cdrh/cfdocs/cfMAUDE/TextSearch.cfm>

'Let's Get it Clear' by Dr Barend ter Haar

One in a series of occasional resumés of aspects in the world of posture and mobility where there are common misconceptions, and myths to be addressed, to help promote better practice. Further items can be found at www.beshealthcare.net. If you are interested in receiving further information on the topic, please contact barend@beshealthcare.net.

Dr ter Haar has been involved in seating and mobility for over 30 years, including lecturing internationally, and developing international seating standards.

